Instrument Manual

ADInstruments

Quad-wavelength laser source AD2Q01F

CONTENTS	PAGE
1 Introduction	3
2 Warranty	4
2.1Three Years Limited Warranty	
2.2 Exclusions	
2.3 Returning Product	
2.4 Contact us	
3 Safety Information	6
4 Preparing for Operation	7
4.1 Unpacking the instrument	
4.2 Power Supply	
5 Operation	9
5.1 Display and controls	
5.2 Turning the instrument on and off	
5.3 Switching the wavelengths	
5.4 Frequency Output	
5.5 Auto-wavelength Recognition	
5.6 Switching backlighting of the LCD of	on and off
5.7 Connecting with Optical Power Met	ter
6 Specifications	19
7 Maintenance	21
8 Trouble shooting	22
©Copyright Abacanto Digital SA.	Manual de usuario AD2Q01F 2



Introduction

The AD2Q0IF quad-wavelength laser source offers excellent stability, portability and facile adjustments for accurate optical fiber testing. Two output connector serves four wavelengths 850nmII300nmII310nmII550nm.

AD2Q0IF can be used to test optical fiber of long distance and local network. Also it can work with optical power meter to measure the loss of optical fiber.

Features:

Easy-to-use, straight forward operation
Eye-catching handheld package
LCD backlight for easy operation in darker environments
Rechargeable battery inside
Three-year warranty and recommended calibration
interval.

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

2. Warranty

Three Years Limited Warranty

Abacanto Digital products are warranted against the defective components and workmanship for a period of three years from the date of delivery to the original customer. Any product found to be defective within the warranty period would be returned to **Abacanto Digital** authorized service center for repair, replacement and calibration.

Exclusions

The warranty on your equipment shall not apply to defects resulting from the following:

Unauthorized repair or modification including battery replacement

Misuse, negligence, or accident

Returning Product

To return product, you may contact Abacanto Digital to obtain additional information if necessary. To serve you better, please specify the reasons for the return.

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

Contact Us

Tel: +34 91 661 30 37 Fax: +34 91 661 49 17

E-mail: info@abacantodigital.com Website: www.abacantodigital.com

3 Safety Information

Warnings!

- Never look directly into optical outputs or a fiber while the equipment is on. Invisible laser beam may damage your eyes.
- Do not short-circuit the terminal of AC adapter I charger and the batteries. Excessive electrical current may cause personal injury due to fumes, electric shock or equipment damage.
- Connect DC power cord with the equipment and wall socket properly. While
 inserting the DC plug, make sure there is no dust or dirt on the terminals and
 both plugs are fully seated. Incomplete engagement may cause fuming,
 electric shock or equipment damage and may result in personal injury.
- Do not operate the equipment near hot objects, in hot environments, in dustyl humid atmosphere or when condensation is present on the equipment. This may result in electric shock, product malfunction or poor performance.

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

ΛD	Inc	trum	onte
AD	ıns	trum	ents

4 Preparing for Operation

4. 1 Unpacking the

Packing material

We suggest that you keep the original packing material. Using the original packing material is your guarantee of protecting the instrument during transit.

Checking the package contents

The standard accessories of **AD2QOIF** are as follows:

- Main unit(including battery)
- Quality Check Report
- DC 6V Adapter

- Carrying Case
- User's Guide

Checking for damage in transit

After unpacking the instrument, check to see whether it was damaged in transit. This is particularly likely if the outer casing is clearly damaged. If there is damage, do not attempt to operate the instrument or to repair it without authorization. Doing so can cause further damage and you may lose your warranty qualification.

©Copyright Abacanto Digital SA. Manual de usuario AD2Q01F 7

ΛD	Inc	trum	onte
AD	ıns	trum	ents

4.2 Power Supply

There are battery indicator and power plug on the screen to show the power supply. When you use the DC 6v charger, there is no battery indicator on the screen. When you do not connect the DC 6v charger, the adapter indicator will disappear on the screen.



When you use the battery, the battery indicator on the screen will show the remaining charge. An empty battery indicator means the power is almost out. When the battery charge is extremely low to supply the necessary power, the instrument will automatically switch off after several beeps of the buzzer. Please change the battery or recharge it



5 Operation

5. 1 Display and

5. **1** . **1** Front(Panel



No.	Key	Function		
I	>2s PERM ON OFF	Switches Instrument on/off. Long keypress while powering on to activate the instrument without Auto-off function.		
2	S/M	Switch between Single Mode and Multimode		
3	CW/Hz	Modulated Wavelength Shifting Key: Switches modulated wavelength and continuous wavelength.		
4	λ	Wavelength Shifting Key: Switches working wavelength between 850nm,I300nm,I310nm and I550nm.		
5	TWIN	SINGLE: Auto-wavelength recognition is off. TWIN: Auto-wavelength recognition is on.		
6	*	Switches backlighting on/off.		

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

5. 1 .2 Back &



Battary Plate (including 2 units of AA recharging batteries)

DC 6v power input

Charging Signal light(Red light blinking means charging, Green light means charging finish).


Standard Accessories:

FC/PC, SC/PC, ST/PC interchangeable connector, Manual, Carrying Bag, and Battery, Worldwide compatible AC/DC adapter, Test Report

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F 10

5.1.3

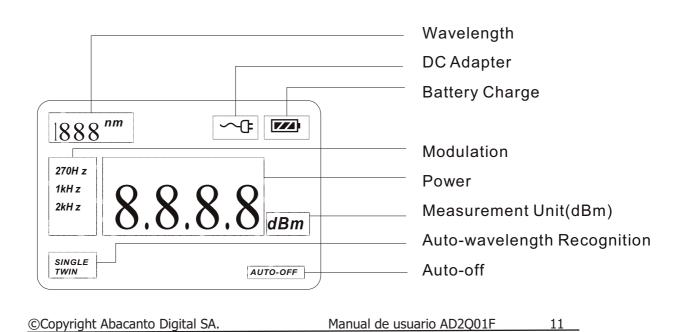

5.2 Turning the instrument on and off



Press the ON/OFF" key briefly.
The instrument powers on. (See the figure)
Press the ON/OFF" key briefly again.
The instrument powers off.



Note: Auto-off function

I The instrument powers off automatically if no key press in I0 minutes. 2 Press the ON/OFF" key for about 2 seconds to power on the instrument with "Auto-off" function deactivated.


©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

5.3 Switching the wavelengths

5.3.1 Switching the wavelengths

Press the to "Mulitimode", then Press \(\lambda\) Key to switch the wavelength between I3IOnm, I55Onm and Off.

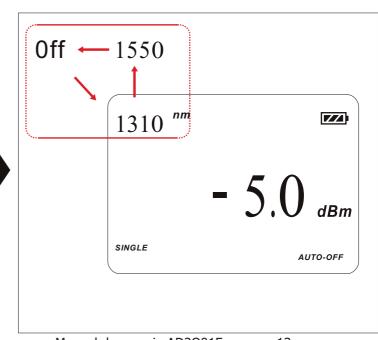


©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

5.3.2 Switching the wavelengths in the in the "Multimode"

Press the sm to "Mulitimode", then Press \(\lambda\) Key to switch the wavelength between 850nm, 1300nm and 0ff.

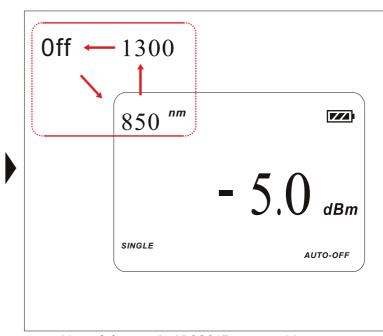

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F


14___

5.4 Frequency Output



The instrument defaults to CW when it switch on. When it is set to CW, there is no frequency on display.

Press the "CW/Hz" Key to select the output among 270Hz, 1kHz and 2kHz.

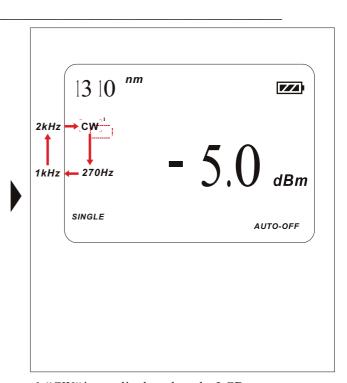

1."CW" is not displayed on the LCD

Manual de usuario AD2Q01F

<u> 15</u>

©Copyright Abacanto Digital SA.

5.5 Auto-wavelength Recognition




Press the "TWIN" Key to tun on and off the auto-wavelength recognition function.

5.6 Switching backlighting of the LCD on and off



Press the backlighting Key to switch the backlighting of the LCD on and off.

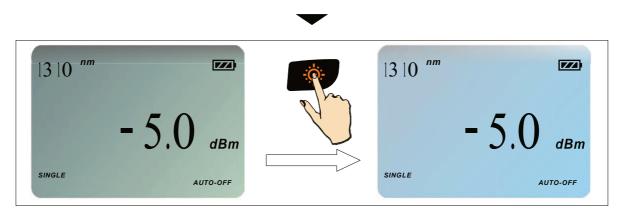

©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

5.7 Connecting with Optical Power Meter

It can work with optical power meter to measure the loss of optical fiber accurately.



©Copyright Abacanto Digital SA.

Manual de usuario AD2Q01F

6 Specifications

Optical Specifications

Model	FHS2Q0 F
Output wavelength (nm)	850/1300/1310/1550
Laser	Class I
Spectral Width	3nm typical value
Stability (15 min preheat @ 25)	±0.05dB/15min ±0.1dB/5hr
CW output power	-5.0dBm±1dB
Modulated Wavelength	270Hz,1kHz,2kHz
Available Connector	FC/PC,SC/PC,ST/PC Interchangeable connectors
Power	2 units of AA recharging battaries
AC Adapter	2Input: AC 100-240V 50/60HZ Output:DC 6V/1A

©Copyright Abacanto Digital SA. Manual de usuario AD2Q01F 19

AD	Instruments	

General Specifications

Operation Temperature	-10°C~+50°C
Storage Temperature	-20°C~+70°C
Humidity	<90%
Size(HXWXD)	160mmx76mmx45mm
Weight	0.27 kg(including batteries)

7 Maintenance

- Please disconnect the DC adapter/charger and cover the protective dust cap once you finish using.
- It is a good idea to clean the connector and the instrument when they get dirty through use. Optical cleaning pads and anhydrous alcohol is recommended. And please be careful not to get the detergent inside the instrument.
- To ensure the measurement accuracy, please send the instrument to our Service Center for calibration once a year.

AD	Instruments	
----	-------------	--

8 Trouble shooting

Malfunction Type	Possible Cause	Recommended solution	Remarks
Failure to turn on/off	No power input	Plug in battery or AC	DIY Available
	Battery exhausted	Charge battery	DIY Available
	Reverse-installed battery	Re-install battery	DIY Available
		(Still doesn't work)	Return to factory
On&off disorder	Low battery	Charge battery or use AC power supply	DIY Available
Inaccurate measurement	Contaminated connector	Swab the dust by using an alcohol-	DIY Available
		impregnated thin cotton swab	
	Connector unfitted	Re-install the connector	DIY Available
Error display	Humid environment	Try later while it is not too humid	DIY Available
	Magnetic field environment	Stay far away from magnetic field	DIY Available
	Metal dust environment	May cause damage on mainboard	Return to factory
	Humid environment	Try later while it is not too humid	DIY Available
On&off failure	Keypad short circuit	Replace keypad	Return to factory

©Copyright Abacanto Digital SA. Manual de usuario AD2Q01F 22